


Corrtest potentiostat /galvanostat / electrochemical workstation Model CS310M consists of DDS arbitrary function generator, high power potentiostat/galvanostat, dual-channel correlation analyzer, dual-channel high-speed 16bit/high-precision 24bit AD converter and extension interfaces. It has more than 40 electrochemical methods including built-in EIS (frequency range 10 μ Hz~1MHz). Max. current is $\pm 2A$, potential range is $\pm 10V$. It can be used for various electrochemical fields such as corrosion, energy, material and electroanalysis. The current can be boosted up to 20A with a current booster, and compliance voltage can be expanded up to 30V, which can meet the needs of power batteries, electrolysis and electrodeposition field.




Application

Corrosion

Corrtest potentiostat includes all the electrochemical techniques for corrosion measurement such as OCP, polarization curve (potentiodynamic), EIS, Cyclic polarization CPP (passivation curve), Electrochemical Potentiokinetic Reactivation (EPR), Hydrogen diffusion test, ZRA, Electrochemical noise, etc. It can be used to study metal corrosion mechanism and corrosion resistance, and evaluate the coating durability and sacrificial anode current efficiency. It can also be used for rapid screening of corrosion inhibitors, fungicides, etc.

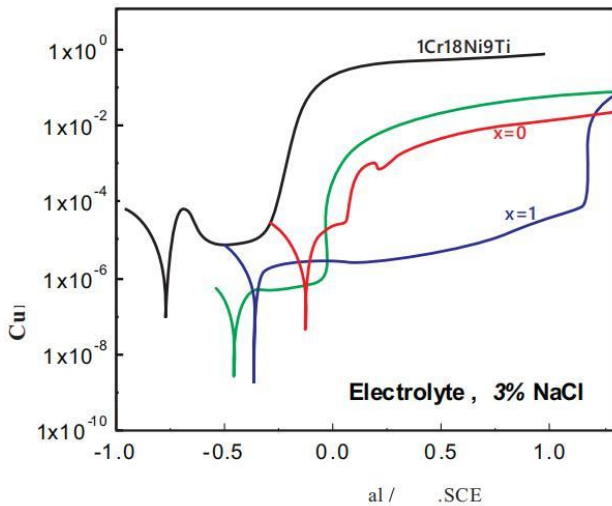


Polarization curves of Ti-alloy& stainless steel in 3%NaCl solution

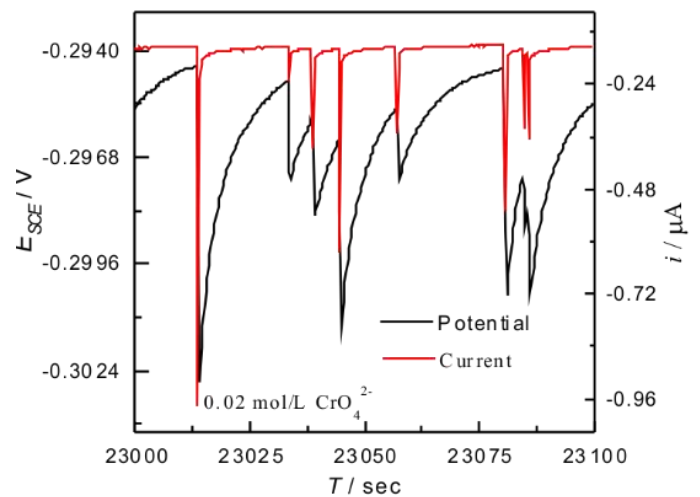

EN of low-carbon steel in 0.05mol/LCl⁻+0.1mol/LNaHCO₃


It uses correlation integral algorithm and dual-channel over-sampling technique, and has strong anti-interference ability. The internal resistance of the instrument is up to 1013 Ω . It's suitable for EIS measurements of high-impedance system (such as coating, concrete etc.)

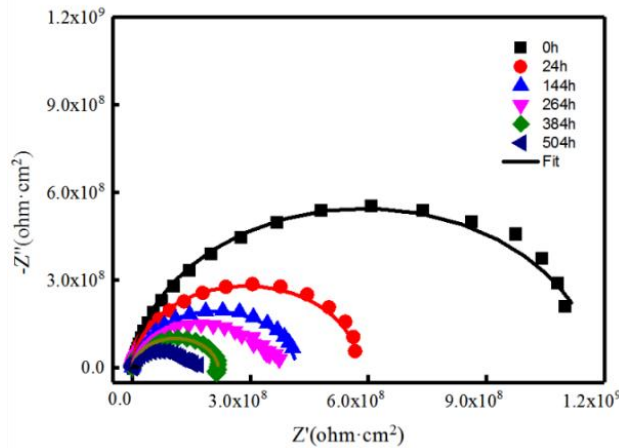

Salt spray aging test of high impedance coating

Energy


With techniques LSV, CV, galvanostatic charge and discharge (GCD), Constant potential/ current EIS, and precise IR compensation circuit, Corrtest potentiostats are widely used in supercapacitor, Li-ion batteries, sodium-ion batteries, fuel cell, Li-S batteries, solar cell, solid-state batteries, flow batteries, metal-air batteries etc. It is an excellent scientific tool for researchers in the fields of energy and materials.

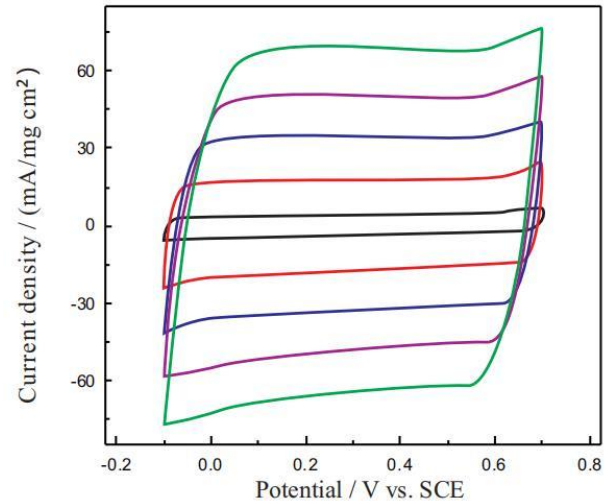

CV curve of PPY supercapacitor in 0.5 mol/L H₂SO₄ solution

Electrocatalysis

- Corrtest potentiostat can measure the half-wave potential (ORR), overpotential (HER, OER) of the catalyst, and has the function of peak power density and energy density calculation.
- Long-term cyclic measurement for ORR, OER, HER, CO₂RR by techniques such as cyclic voltammetry, potentiostatic, galvanostatic. Faraday efficiency can be measured with a bipotentiostat.
- Maximum current can be 20A and compliance voltage can be 30V, and with IR compensation technique, Corrtest potentiostat can precisely measure the overpotential of the electrode, which is a big advantage in electrocatalysis field.

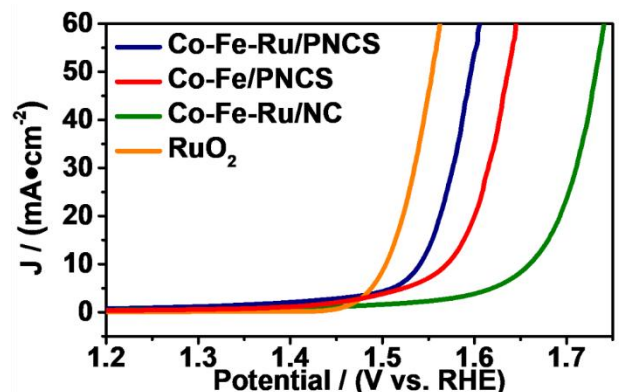

LSV curve of catalysts in alkaline solution

Sensors

CS100 handheld potentiostat can be used in the field of biosensors and chemical sensors, and many others. With the size of a mobile phone, it can be carried easily for lab and on-site use. Potential resolution is 3 μ V, and current resolution can be 1pA.

Advantages

Full floating


All Corrttest potentiostats / galvanostats are designed as full-floating, and can be used for electrochemical study of working electrode connecting to earth, such as autoclave, metal part in bridge, concrete

EIS

- Corrttest potentiostat uses correlation integral algorithm and dual-channel over-sampling technique, and has strong anti-interference ability. The internal resistance of the instrument is up to 1013Ω . It's suitable for EIS measurements of high-impedance system (such as coating, concrete etc.)
- With constant current carrier and DC bias technology, Corrttest potentiostat can be used for battery impedance measurement under charge and discharge state, suitable for ultra-low resistance system (such as 18650 battery, soft pack battery, battery core...)

Multi electrode system

- Support 2-, 3-, 4-electrode system, can be used to test battery inter measurement
- With Zero resistance ammeter for galvanic current measurement

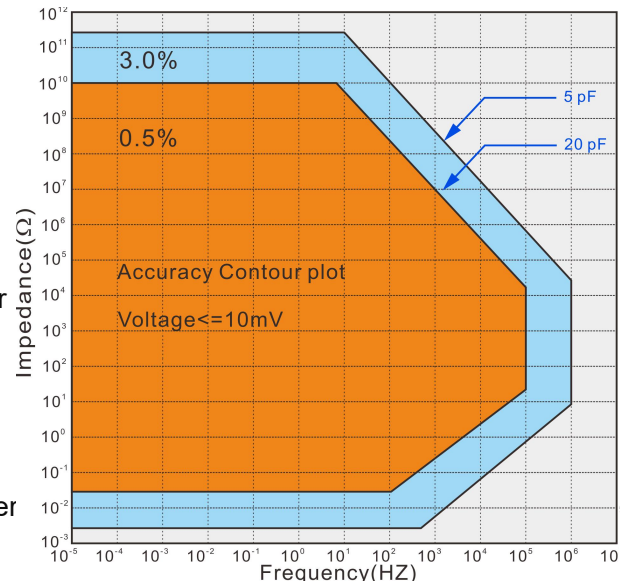

EIS Accuracy

Combination test

CS studio software supports the combination test for various experiments to achieve flexible and unattended test. You can set the parameters for each experiment in advance, and set the intervals, wait time etc between each experiment.

No.	Name	Description
1	Start time	The following test starts at [2022/03/23 11:34:35]
2	Start the cycle	Cycles:3
3	Open Circuit Potential	Freq(Hz):10, Hold Time(s):1800
4	Potentiostatic EIS (IMP)	DC Potential(V):0, Amplitude(mV):10, Initial Frequency:100000, Final
5	Potentiodynamic (Tafel, LPR)	Init E(V):-0.1 vs OCP, Final E(V):0.1 vs OCP, Scan Rate(mV/s):0.5, Freq
6	Wait	After 180 seconds, testing will be continued
7	End the cycle	End

Combination Test: corrosion tests

No.	Name	Description
1	Cyclic Voltammetry	Step1 E(V):-1 vs Ref, Step2 E(V):1 vs Ref, Scan Rate(mV/s):5, Freq(Hz):10, Cycl
2	Cyclic Voltammetry	Step1 E(V):-1 vs Ref, Step2 E(V):1 vs Ref, Scan Rate(mV/s):10, Freq(Hz):20, Cyc
3	Cyclic Voltammetry	Step1 E(V):-1 vs Ref, Step2 E(V):1 vs Ref, Scan Rate(mV/s):20, Freq(Hz):40, Cyc
4	Cyclic Voltammetry	Step1 E(V):-1 vs Ref, Step2 E(V):1 vs Ref, Scan Rate(mV/s):50, Freq(Hz):100, C
5	Cyclic Voltammetry	Step1 E(V):-1 vs Ref, Step2 E(V):1 vs Ref, Scan Rate(mV/s):100, Freq(Hz):200, C
6	Cyclic Voltammetry	Step1 E(V):-1 vs Ref, Step2 E(V):1 vs Ref, Scan Rate(mV/s):200, Freq(Hz):400, C
7	Cyclic Voltammetry	Step1 E(V):-1 vs Ref, Step2 E(V):1 vs Ref, Scan Rate(mV/s):500, Freq(Hz):1000

Combination Test: Pseudo capacitor tests


High current option

- With the booster, the current can be boosted to 20A, which meets the requirement in fuel cell, power battery, electroplating, etc
- Can customize the instrument to be 30V high compliance voltage, which meets the test requirement in low-conductivity solutions (organic system, concrete system etc), especially suitable for carbon and nitrogen reduction study.



Software development kit(SDK)

We can provide secondary development interfaces, API general interfaces and development examples, and can realize data call for Labview, C, C++, C#, VC and other program, which is convenient for secondary development and test methods customization.

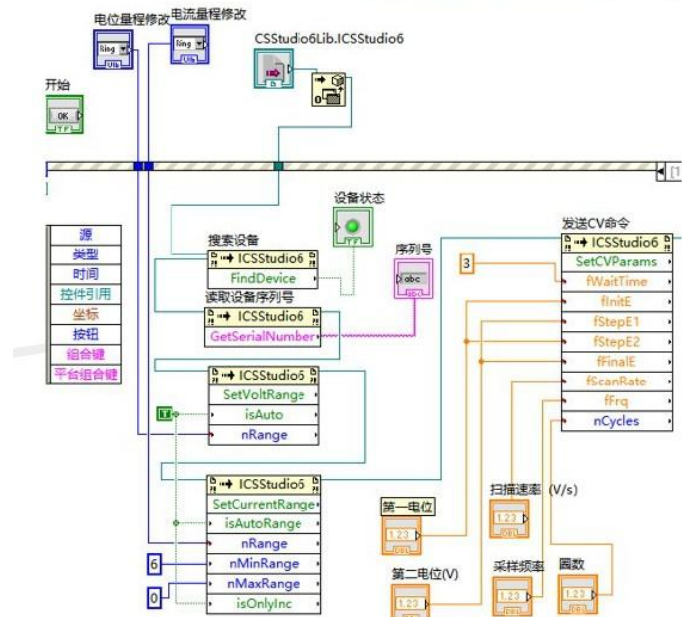


Real-time data storage

Experiment data can be stored in real time. Even if the test is interrupted by a power failure, the data will be automatically saved. The data is compatible with Excel, Origin, and can be directly opened in third-party software for data processing and curve drawing.

Versatile data analysis

CS Studio is the software for Corrttest potentiostat for experiment control and data analysis. It can do: multi-parameter Tafel curve fitting, derivation, integration and peak height analysis of voltammetric curve, EIS equivalent circuit customization and impedance spectrum fitting, etc.

- Multi-parameters Polarization curve
- EIS fitting
- Electrochemical noise analysis
- Pseudocapacitance calculation
- GCD specific capacitance, efficiency
- Mott-Schottky plot analysis
- CV analysis

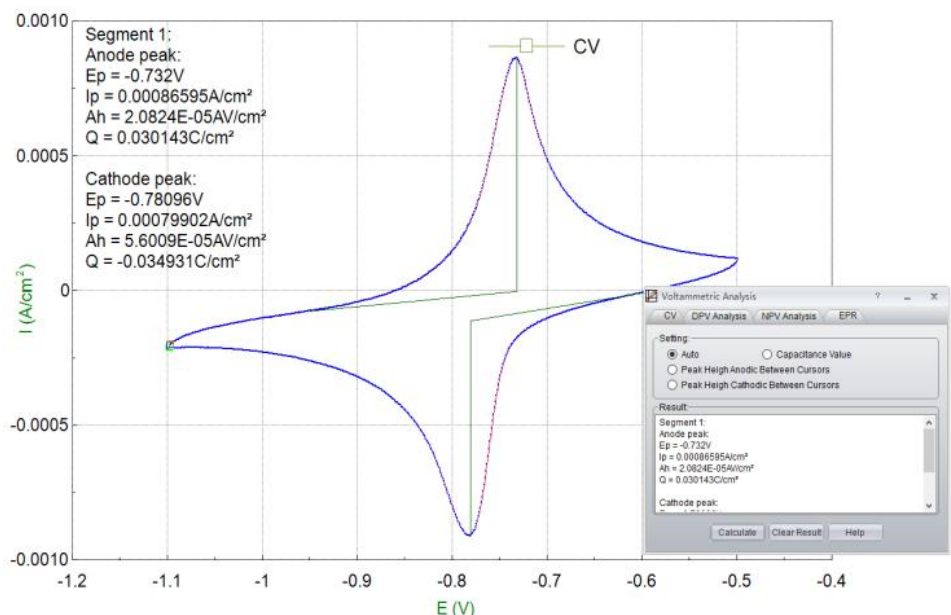

Specifications

Specifications	
Support 2-, 3- or 4-electrode system	Potential and current range: Automatic
Potential control range: $\pm 10V$	Current control range: $\pm 2A$
Potential control accuracy: $0.1\% \times \text{full range} \pm 1mV$	Current control accuracy: $0.1\% \times \text{full range}$
Potential resolution: $10\mu V$ ($>100Hz$), $3\mu V$ ($<10Hz$)	Current sensitivity: $1pA$
Rise time: $<1\mu S$ ($<10mA$), $<10\mu S$ ($<2A$)	Reference electrode input impedance: $10^{12}\Omega 20pF$
Current range: $2nA \sim 2A$, 10 ranges	Compliance voltage: $\pm 21V$
Maximum current output: $2A$	CV and LSV scan rate: $0.001mV \sim 10,000V/s$
CA and CC pulse width: $0.0001 \sim 65,000s$	Current increment during scan: $1mA @ 1A/ms$
Potential increment during scan: $0.076mV @ 1V/ms$	SWV frequency: $0.001 \sim 100 kHz$
DPV and NPV pulse width: $0.0001 \sim 1000s$	AD data acquisition: $16bit @ 1 MHz, 20bit @ 1 kHz$
DA Resolution: $16bit$, setup time: $1\mu s$	Minimum potential increment in CV: $0.075mV$
IMP frequency: $10\mu Hz \sim 1MHz$	Low-pass filters: covering 8-decade
Operating System: Windows 2000/NT/XP/ 7/8/10	Interface: USB 2.0
Weight / Measurements: $6.5kg, 36.5 \times 30.5 \times 16 cm$	
EIS (Electrochemical Impedance Spectroscopy)	
Signal generator	
Frequency range: $10\mu Hz \sim 1MHz$	AC amplitude: $1mV \sim 2500mV$
DC Bias: $-10 \sim +10V$	Output impedance: 50Ω
Waveform: sine wave, triangular wave and square wave	Wave distortion: $<1\%$
Scanning mode: logarithmic/linear, increase/decrease	
Signal analyzer	
Integral time: minimum: $10ms$ or the longest time of a cycle	Maximum: 10^6 cycles or 10^5s
Measurement delay: $0 \sim 10^5s$	
DC offset compensation	
Potential automatic compensation range: $-10V \sim +10V$	Current compensation range: $-1A \sim +1A$
Bandwidth: 8-decade frequency range, automatic and manual setting	

Techniques / Software - Model CS310M

Stable polarization

- Open Circuit Potential (OCP)
- Potentiostatic (I-T curve)
- Galvanostatic
- Potentiodynamic (Tafel plot)
- Galvanodynamic (DGP)
- Sweep-Step Functions (SSF)

Transient Polarization

- Multi Potential Steps
- Multi Current Steps
- Potential Stair-Step (VSTEP)
- Galvanic Stair-Step (ISTEP)

Chrono Method

- Chronopotentiometry (CP)
- Chronoamperometry (CA)
- Chronocoulometry (CC)

Voltammetry

- Linear Sweep Voltammetry (LSV)
- Cyclic Voltammetry (CV)

Electrochemical Impedance Spectroscopy (EIS)

- EIS vs Frequency (IMP)
- Galvanostatic EIS
- EIS vs Potential (IMPE)(Mott-Schottky)
- EIS vs Time (IMPT)
- Galvanostatic EIS vs Time

Corrosion Measurements

- Cyclic polarization curve (CPP)
- Linear polarization curve (LPR)
- Electrochemical Potentiokinetic Reactivation (EPR)
- Electrochemical Noise (EN)
- Zero resistance Ammeter (ZRA)

Battery test

- Battery Charge and Discharge
- Galvanostatic Charge and Discharge (GCD)
- Potentiostatic Charging and Discharging (PCD)
- Potentiostatic Intermittent Titration Technique (PITT)
- Galvanostatic Intermittent Titration Technique (GITT)

Extensions

- Electrochemical Stripping/ Deposition
- Bulk Electrolysis with Coulometry (BE)
- Rs Measurement

Software Features


Cyclic voltammetry:

CS studio software provides users a versatile smoothing/differential/ integration kit, which can complete the calculation of peak height, peak area and peak potential of CV curves. In CV technique, during the data analysis, there is function of selecting exact cycle(s) to show. You can choose to see a cycle or some cycles as you want. You can also export data or vector graph of an exact cycle or several cycles.

Tafel plot and corrosion rate:


CS studio also provides powerful non-linear fitting on Butler-Volmer equation of polarization curve. It can calculate Tafel slope, corrosion current density, limitation current, polarization resistance, corrosion rate. It can also calculate the

power spectrum density, noise resistance and noise spectrum resistance based on the electrochemical noise measurements.

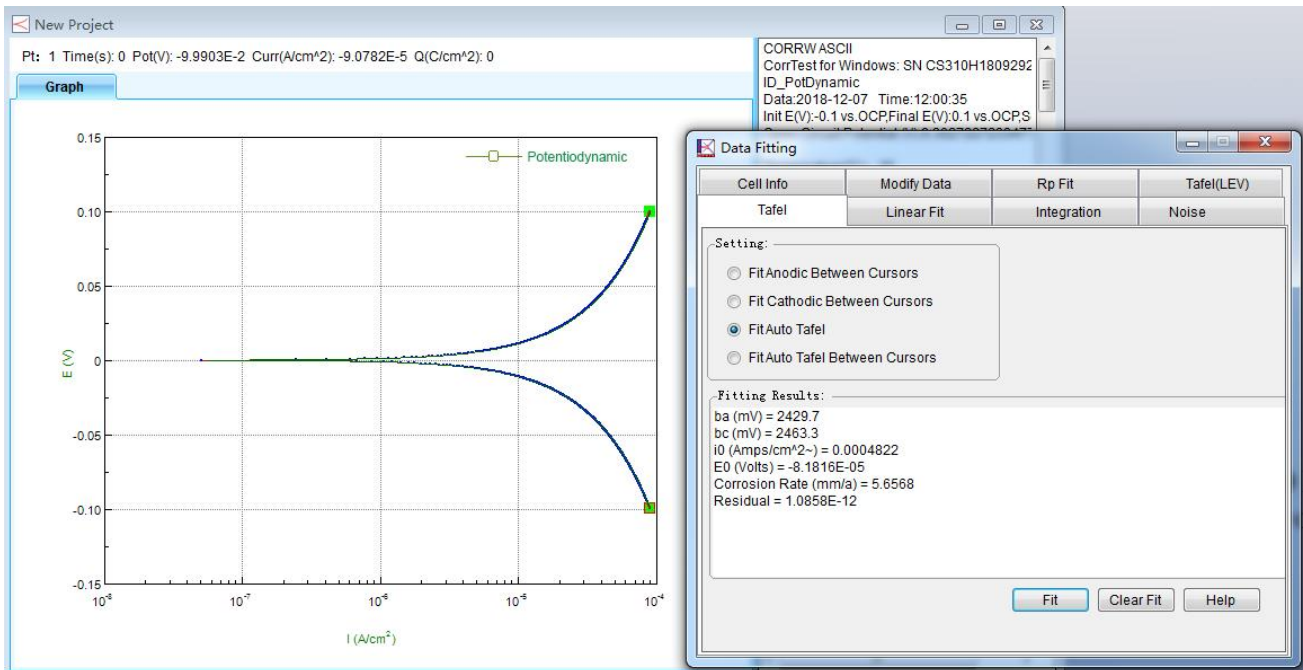


Battery Test and analysis:

charge & discharge efficiency, capacity, specific capacitance, charge & discharge energy.

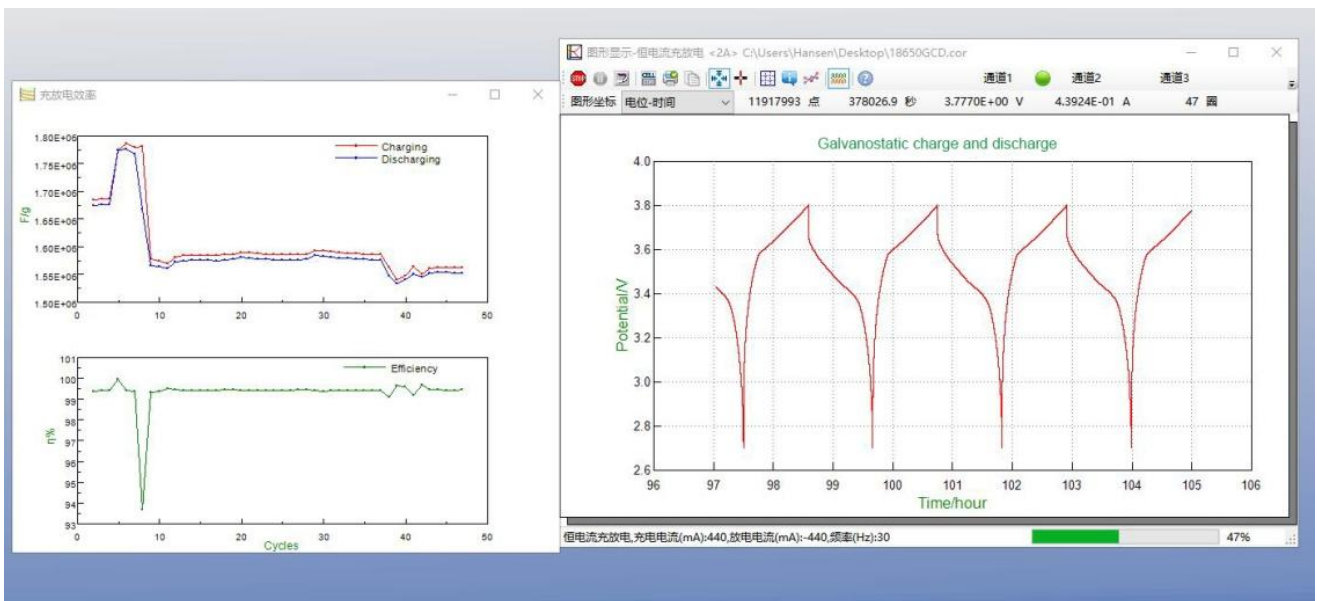

EIS analysis: Bode, Nyquist, Mott-Schottky plot

During EIS data analysis, there is built-in fitting function to draw the custom equivalent circuit.

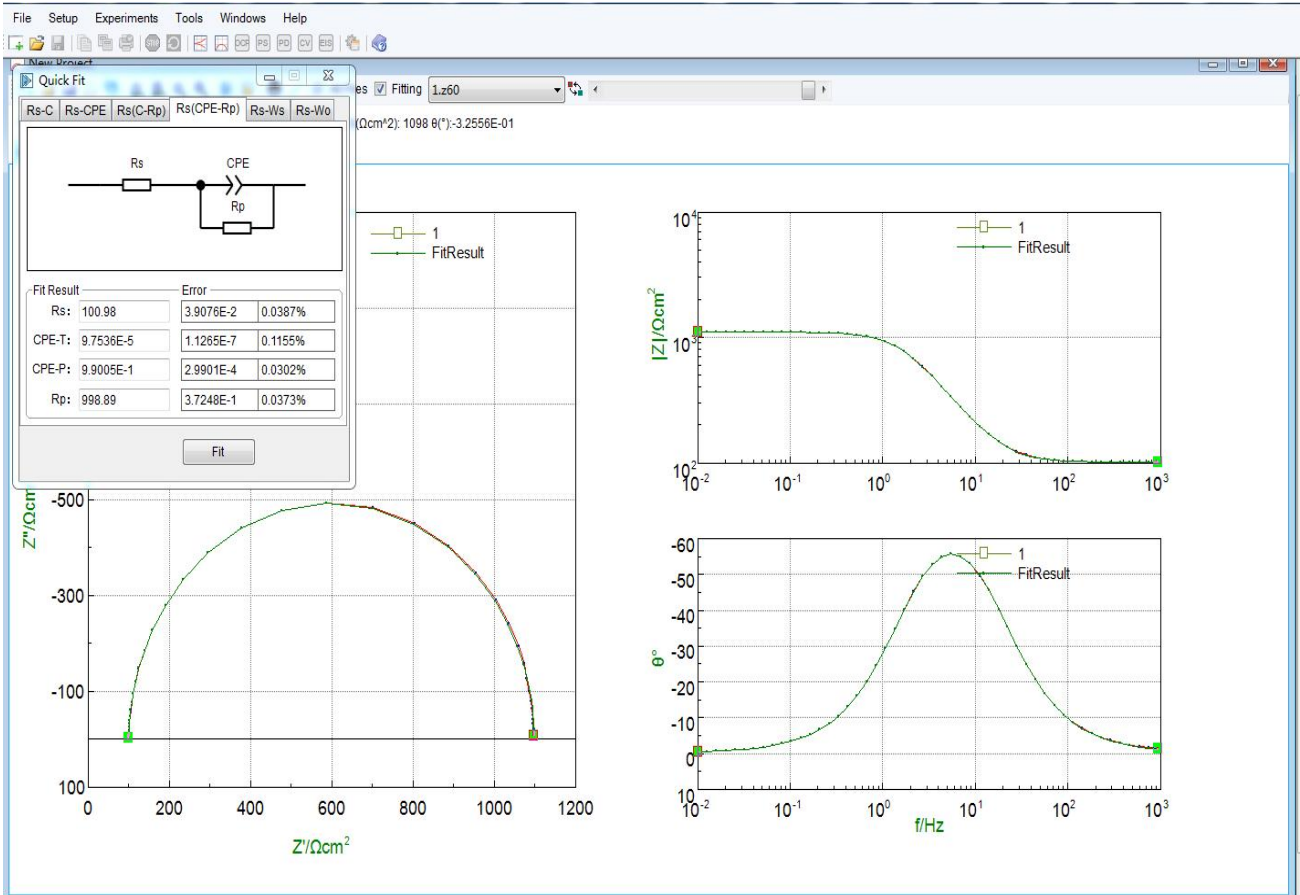

Standard supply list for each set

- Instrument host CS310M x1
- CS studio software x1
- Power cable x1
- USB cable x1
- Cell cable x2
- Dummy cell(1k Ω ||100 μ F) x1
- Manual x1

Service: (**all the service is free)

1. Warranty period: 5 years
2. Provide installation guidance and manual, software installation video.
3. Lifetime free software upgrading and technical service
4. Provide repair service for free

Contact us

Wuhan Corrtest Instruments Corp., Ltd.

Add: #505, Jinfeng Bld. A, International Enterprise Center,
Optics valley Ave., East lake High-tech Dev. Zone, Wuhan city, 430074, China

Email: sales2@corrtest.com.cn

Mob./whatsapp: +86 13469965984

Website: <https://www.corrtestinstruments.com/en>
<http://www.corrtest.com.cn/en>